


IMPRESSIONS

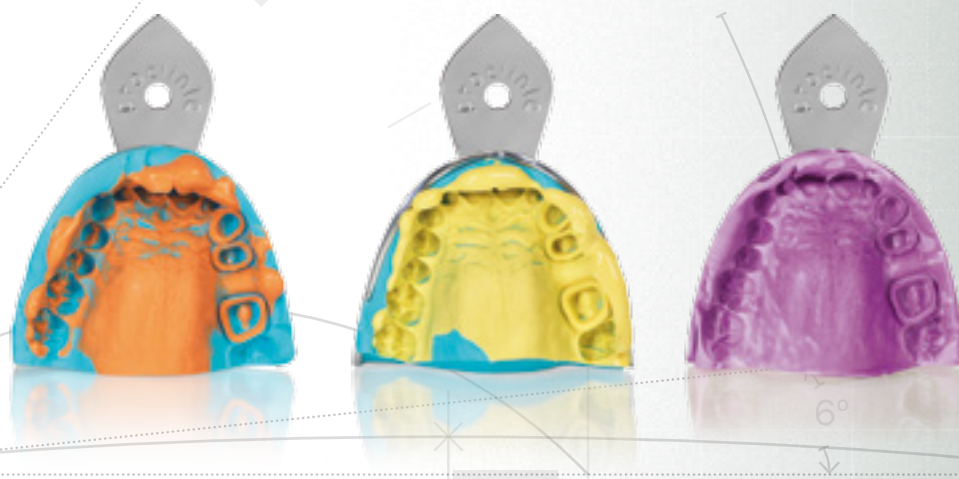

INCREDIBILMENTE EASY AND ACCURATE

For any technique:
1-step, 2-step and monophasic

Proclinc Expert silicones guarantee maximum precision and quality

Nanotechnology and hydrophilic properties combine to provide detailed impressions, guaranteed dimensional precision and total margin integrity.




Excellent reproduction of details

Highly hydrophilic, contact angle < 10°

High elasticity and tear resistance

Versatile, can be used in 1 or 2-step and monophasic techniques

Perfect thixotropy, no bubbles or drips

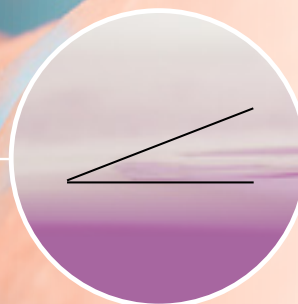

Dr. Alexander Johansson

Clínica ZahnCity GmbH, Zurich, Switzerland
www.zahncity.ch

"I had not tried an ultralight silicone before and I have found that Proclinic Expert Ultra Light Body silicone is better than the light body silicone I usually use."



Dr. Eduardo González Arroyo

Clínica Fernández, Ibiza, Spain
www.oralsturgerytube.com
Member of Association of Dental Surgeons number 28007247

"These new silicones are better quality than the previous generation of Proclinic silicones which I always used in the past."

Proclinic Expert
silicones are
recommended by
professionals:



Dr. Carlos Gargallo

Clínica Carlos Gargallo,
Barcellona, Spain
Member of Association of Dental Surgeons number 3947


"The Proclinic Expert range of silicones provides very satisfactory results in all customary impression techniques. Both the normal and ultra-light products offer a very high degree of precision and consistency and are easy to handle; they are ideal for fixed dentures, invisible braces and rebases. After a double impression, manual silicone putties and automatic mix putties can be trimmed easily with a scalpel."



Proclinic Expert silicones allow impressions to be taken quickly and easily

Modulated times and different viscosities for each and every clinical need.
Details reproduced accurately.

Highly hydrophilic, minimising the risk of pores. Ensure highly accurate impressions by using Proclinic Expert silicones.

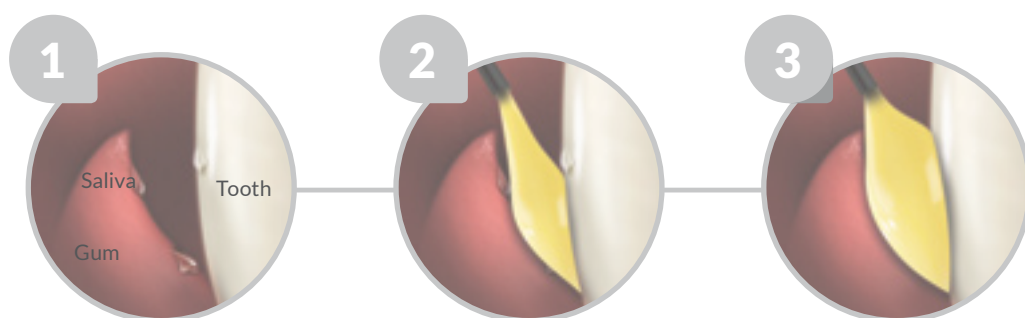

*Times at 23° C	Ultra Light Body	Light Body	Light Body	Regular Body	380 Heavy Body	380 Heavy Body	380 Putty Soft	Putty Soft	Putty Soft
	Fast Set	Regular Set	Fast Set	Regular Set	Regular Set	Fast Set	Fast Set	Regular Set	Fast Set
Reorder	15156	15153	15154	15152	15158	15159	15157	15150	15151
ISO 4823	Type 3	Type 3	Type 3	Type 2	Type 1	Type 1	Type 0	Type 0	Type 0
ADA 19	Light-bodied Consistency	Light-bodied Consistency	Light-bodied Consistency	Medium-bodied Consistency	Heavy-bodied Consistency	Heavy-bodied Consistency	Putty Consistency	Putty Consistency	Putty Consistency
Mix	1:1	1:1	1:1	1:1	5:1	5:1	5:1	1:1	1:1
System									
Mix type	Auto mixing system	Auto mixing system	Auto mixing system	Auto mixing system	Auto mixing system	Auto mixing system	Auto mixing system	Hand mixing	Hand mixing
Total working time	1'30"	2'	1'30"	2'	2'	1'30"	1'30"	2'	1'30"
Minimum time in patient's mouth	2'30"	3'30"	2'30"	3'30"	3'30"	2'30"	2'30"	3'30"	2'30"
Curing time*	4'	5'30"	4'	5'30"	5'30"	4'	4'	5'30"	4'
Deformation under pressure (min - max)	3 - 5%	3 - 5%	3 - 5%	3 - 5%	3 - 5%	3 - 5%	1- 3%	1- 3%	1- 3%
Elastic memory	> 99,5%	> 99,5%	> 99,5%	> 99,5%	> 99,5%	> 99,5%	> 99%	> 99%	> 99%
24-hour linear dimensional change	< 0,20%	< 0,20%	< 0,20%	< 0,20%	< 0,20%	< 0,20%	< 0,20%	< 0,20%	< 0,20%
Shore A hardness scale	45±2	45±2	45±2	45±2	60±2	60±2	60±2	60±2	60±2
Suggested techniques	2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step	1-step, 2-step
	LOW CONSISTENCY							HIGH CONSISTENCY	

Complete your range of bite registration silicones with Proclinic Expert silicone.
Shore A hardness 95 (15160) guarantees excellent reproduction of details.

Proclinic Expert silicones can be adapted to all impression techniques



1-STEP TECHNIQUE

PUTTY SOFT FAST	Working time 1'30"	Minimum time in mouth 2'30"
LIGHT BODY FAST	Working time 1'30"	Minimum time in mouth 2'30"



2-STEP TECHNIQUE

PUTTY SOFT REGULAR	Working time 2'	Minimum time in mouth 3'30"
ULTRA LIGHT BODY	Working time 1'30"	Minimum time in mouth 2'30"

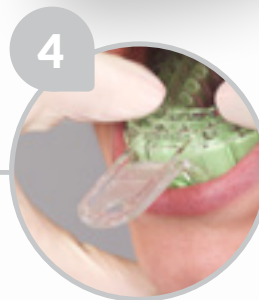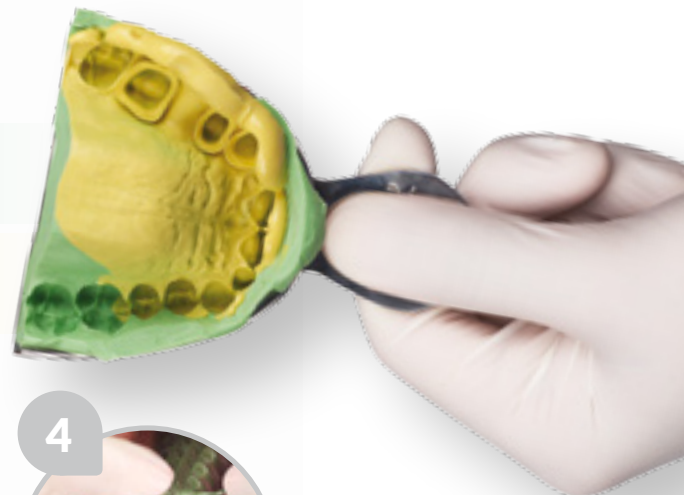

Proclinic Expert silicones guarantee outstanding results in clinical testing



THE DENTAL
ADVISOR
Improving Patient Care Through Research & Education

Proclinic Expert VPS
Impression Material
++++ ½

THE DENTAL ADVISOR
www.dentaladvisor.com

RATINGS:
Excellent +++++
Very Good ++++
Good +++

373
APPLICATIONS



87%

of dentists rate Proclinic
Expert silicones

**AS GOOD AS
OR BETTER**

than their usual silicone



| www.proclinic-products.com |

info@proclinic-products.com |



 **proclinic**
EXPERT